

FUJI SILYSIA CHEMICAL

CHROMATOREX

Technical Bulletin

ARG SILICA

For HILIC compounds



INTRODUCTION

For Hydrophilic Interaction Chromatography compounds

Hydrophilic compounds have been separated in reversed-phased (RP) mode by using media such as C18 (ODS) silica gel in combination with aqueous solvent mixtures. However, there are still many high hydrophilic compounds which cannot be separated using typical RP mode.


Recently, a technique of Hydrophilic Interaction Chromatography (HILIC) has been developed and it is possible to separate high hydrophilic compounds.

Fuji Silysia Chemical Ltd. (FSC) developed "ARG Silica" for HILIC mode (Patent applied in Japan). ARG Silica can separate hydrophilic compounds such as amino acid, peptide, vitamin and nucleic acid.

Various particle size of ARG Silica are available for analysis and large scale purification. ARG Silica is dedicated to the separation of various hydrophilic compounds.

ARG SILICA

ARG Silica is based on a chemical surface modification with arginine amino acid. ARG Silica has strong affinity to hydrophilic compounds and generates high separation performance and different selectivity compared with other grades.

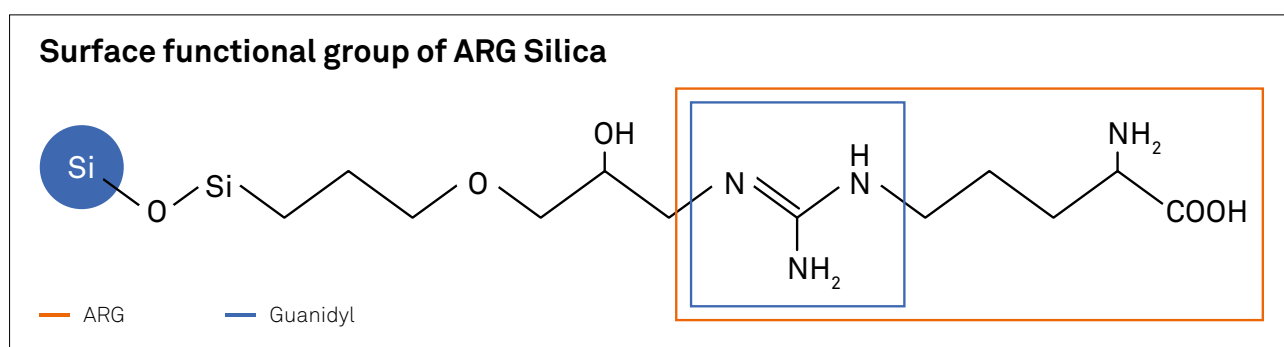

ARG Silica has a "guanidyl" function, improving the hydrophilicity of the media. In HILIC mode, mainly acetonitrile/water mixtures are first choice for mobile phase. High polarity elutes are strongly retained to ARG Silica by hydrophilic interaction. As water content increases, elution time is getting shorter. Thus, separation pattern of ARG Silica is opposite of RP mode where retention time is getting longer as water content increases.

HOW TO USE

It is necessary to flush the column by 70% acetonitrile / water or mobile phase for 10 times higher than column volume to equilibrate column separation layer for preparation before using. If separation was operated with insufficient condition, separation property would be unstable.


Recommendable water content in mobile phase is less than 30 %.

Separation layer would be unstable if higher water content in mobile phase is used. Also if water content between injection solution and mobile phase has big difference, separation peak pattern would be degraded. Thus, the smallest difference of water content between mobile phase and injection solution is recommended.

MOBILE PHASE



More than 4 % water content in mobile phase is recommended to take advantage of HILIC's separation property. Acetonitrile, Isopropanol, Methanol and Water can be applied as mobile phase. As shown in below chromatogram, elution power of acetonitrile is weak, while elution power of water is strong. In general, acetonitrile / water system is used as mobile phase. Effective range of pH for mobile phase is pH 2.0 ~ 9.0.

COMPOSITION OF MOBILE PHASE

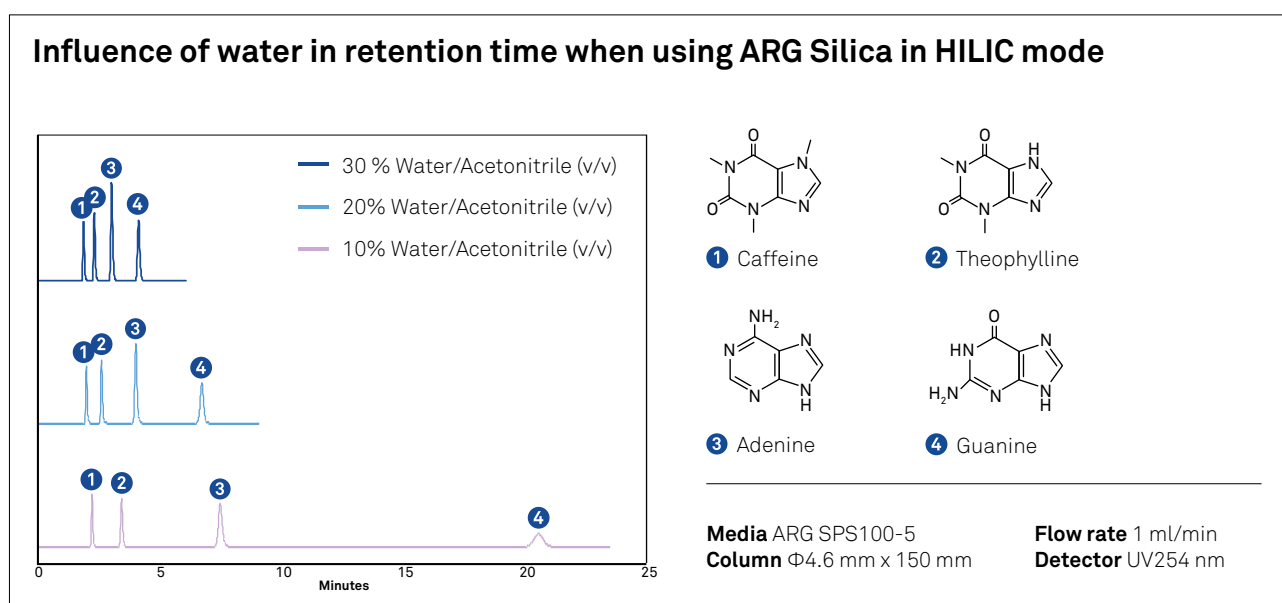


COMPARATIVE DATA BETWEEN ARG SILICA, NH, DIOL AND BARE SILICA

ARG Silica is more effective for the separation of nucleobases and purine bases than NH Silica, Diol Silica and bare Silica. The added guanidyl function improves the hydrophilicity of ARG Silica.

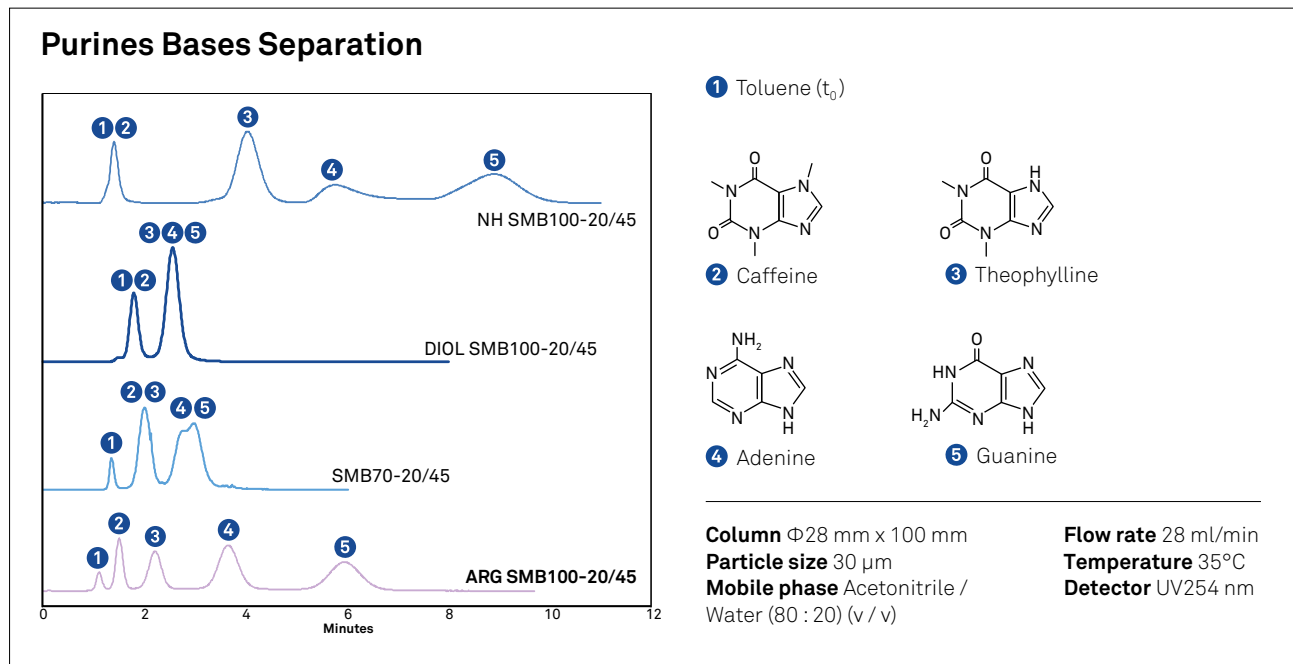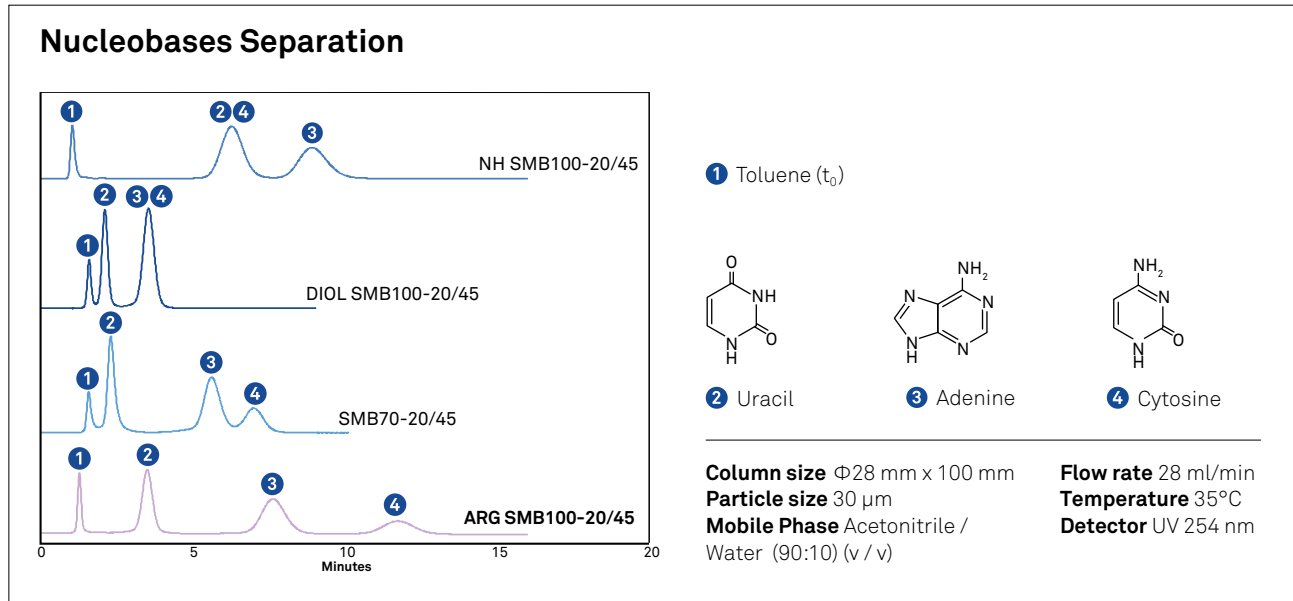

SEPARATION OF HYDROPHILIC COMPOUNDS

1. Separation of polypeptides

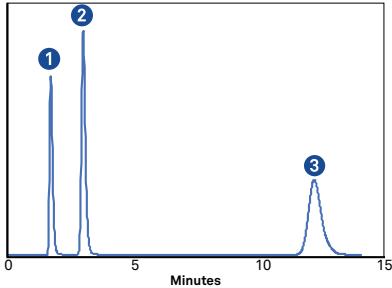

- 1 Angiotensin III
- 2 Bradykinin
- 3 Angiotensin II

Amino acid sequence


- 1 (Arg-Val-Tyr-Ile-His-Pro-Phe)
- 2 (Arg-Pro-Pro-Gly-Phe-Ser-Pro-Phe-Arg)
- 3 (Asp-Arg-Val-Tyr-Ile-His-Pro-Phe)

Media ARG SPS100-5
Column Φ 4.6 mm x 250 mm

Mobile phase
Methanol / Acetonitrile /
50mM Ammonium Acetate
pH6.8 (60:20:20) (v/v)

Flow rate 1 ml/min
Temperature 35°C
Detector UV220 nm

2. Separation of oligopeptides

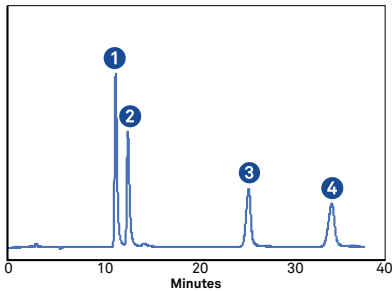



- 1 Gly-Phe
- 2 Gly-Leu
- 3 Gly-Gly
- 4 Gly-Gly-Gly

Media ARG SPS100-5
Column Φ 4.6 mm x 250 mm


Mobile Phase
Acetonitrile / 50mM Tris-HCl
pH=8.5 (70:30) (v/v)

Flow Rate 1 ml/min
Temperature 35°C
Detector UV220 nm


3. Separation of amino acids

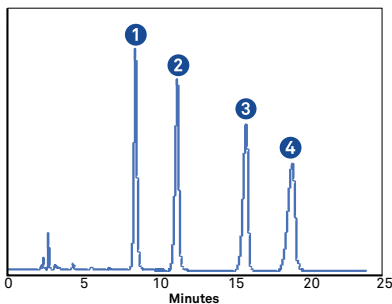

1 L- Leucine



2 L- Valine



3 L- Alanine




4 Glycine

Media ARG SPS100-5
Column Φ 4.6 mm x 250 mm

Mobile Phase
Acetonitrile / Water
(75:25) (v/v)

Flow Rate 1 ml/min
Temperature 35°C
Detector UV210 nm

4. Separation of vitamins

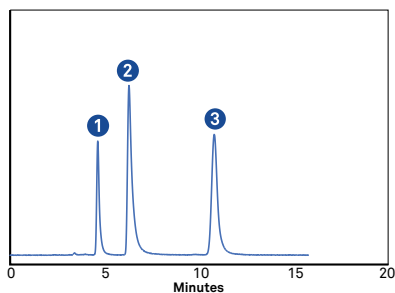



- 1 Riboflavin (Vitamin B₂) 2 Thiamine (Vitamin B₁) 3 Cyanocobalamin (Vitamin B₁₂)

Media ARG SPS100-5
Column Φ4.6 mm x 250 mm


Mobile Phase
Acetonitrile / 50mM Tris-HCl
pH=8.5 (70:30) (v/v)

Flow Rate 1 ml/min
Temperature 35°C
Detector UV254 nm


5. Separation of sugar alcohols

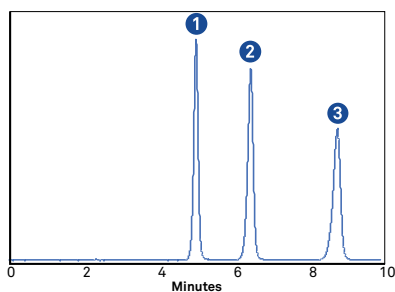

- 1 Erythritol



- 2 Xyritol





- 3 Mannitol

Media ARG SPS100-5
Column Φ4.6 mm x 150 mm


Mobile Phase
Acetonitrile / Water
(80:20) (v/v)

Flow Rate 1 ml/min
Temperature 35°C
Detector ELSD


6. Separation of catecholamines

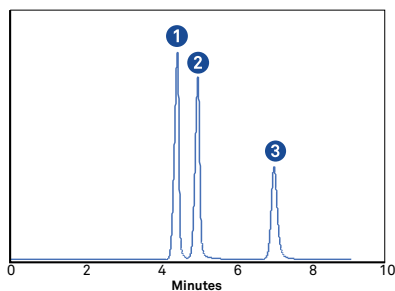

- 1 Dopamine



- 2 Adrenaline




- 3 Noradrenaline

Media ARG SPS100-5
Column Φ4.6 mm x 150 mm

Mobile Phase
Acetonitrile / 50mM
Ammonium formate pH=3.5
(85:15) (v/v)

Flow Rate 1 ml/min
Temperature 35°C
Detector UV270 nm

7. Separation of monosaccharides and disaccharides

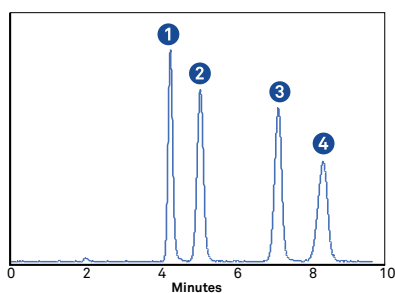

- 1 Fructose 2 Glucose 3 Sucrose 4 Maltose

Media ARG SPS100-5
Column Φ4.6 mm x 150 mm


Mobile Phase
Acetonitrile / Water
(75:25) (v/v)

Flow Rate 1 ml/min
Temperature 60°C
Detector ELSD


Separation of nucleic acid bases by TLC

ARG TLC

UV254 nm




Acetonitrile / Water
(90:10) (v/v)

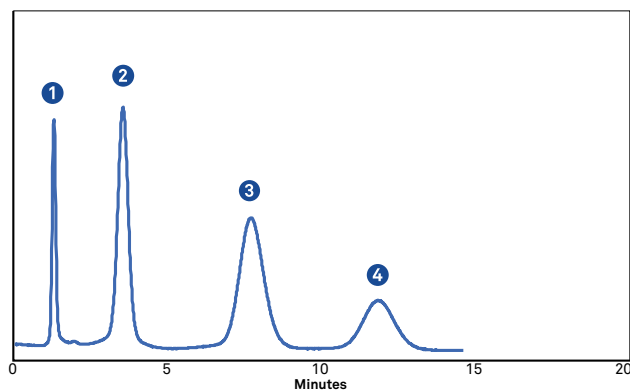


Media ARG SMB100-20/45
Column Φ 28 mm x 100 mm
Mobile Phase Acetonitrile / Water
(90:10) (v/v)

Flow Rate 28 ml/min
Temperature 35°C
Detector UV254 nm


1 Toluene (t_0)



2 Uracil



3 Adenine



4 Cytosine


Separation of Heterocyclic compounds by TLC

ARG TLC

UV254 nm




Acetonitrile / Water
(90:10) (v/v)

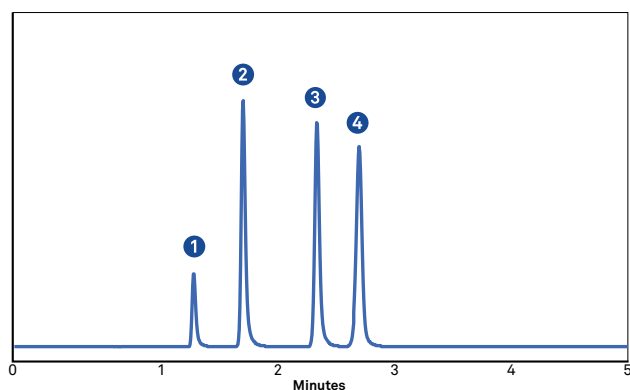


Media ARG SPS100-3
Column Φ 3.0 mm x 150 mm
Mobile Phase Acetonitrile / Water
(90:10) (v/v)

Flow Rate 0.50 ml/min
Temperature 35°C
Detector UV254 nm


1 Toluene (t_0)



2 Caffeine



3 Nicotinamide



4 Theophylline

PRODUCT INFORMATION

Bare Silica :

10nm (100 Å), with 3, 5, 10, 20/45, and 40/75 μ m

Packaging 100g, 1kg, 20kg

TLC Plates :

Glass Plates 20 x 20 cm

Packaging 10 pieces/box



FUJI SILYSIA CHEMICAL LTD.

Head Office
2-1846 Kozoji-cho,
Kasugai-shi,
Aichi-Ken
Japan 487-0013

FUJI SILYSIA CHEMICAL LTD.

Sales Office
23rd floor, Nagoya Intl. Center Bldg.
1-47-1 Nagono,
Nakamura-Ku,
Nagoya-shi,
Aichi-Ken
Japan 450-0001

Phone: +81 52 587 0451

Fax: +81 52 587 0455

E-mail: chromato-int@fuji-silysia.co.jp

FUJI SILYSIA CHEMICAL S.A.


International Chromatography Center
En Budron E9
CH-1052 Le Mont-sur-Lausanne
Switzerland

Phone: +41 21 652 3436

Fax: +41 21 652 4737

E-mail: info@chromatorex.com

www.chromatorex.com



We accept no responsibility for the information offered within this text. We offer this information for the consideration of our customers, but we cannot guarantee the accuracy of the information. Customers are advised to make their own tests to determine the effectiveness and safety of the products described within. Unless otherwise stated in writing in conjunction with our conditions of sale, we supply products without warranty; customers assume all responsibility and liability for any loss or damage resulting from handling or use of our products, whether they are used alone or in conjunction with other products. No statement contained within is intended for any use that violates or infringes any statutory obligation or right which belongs to a third party.